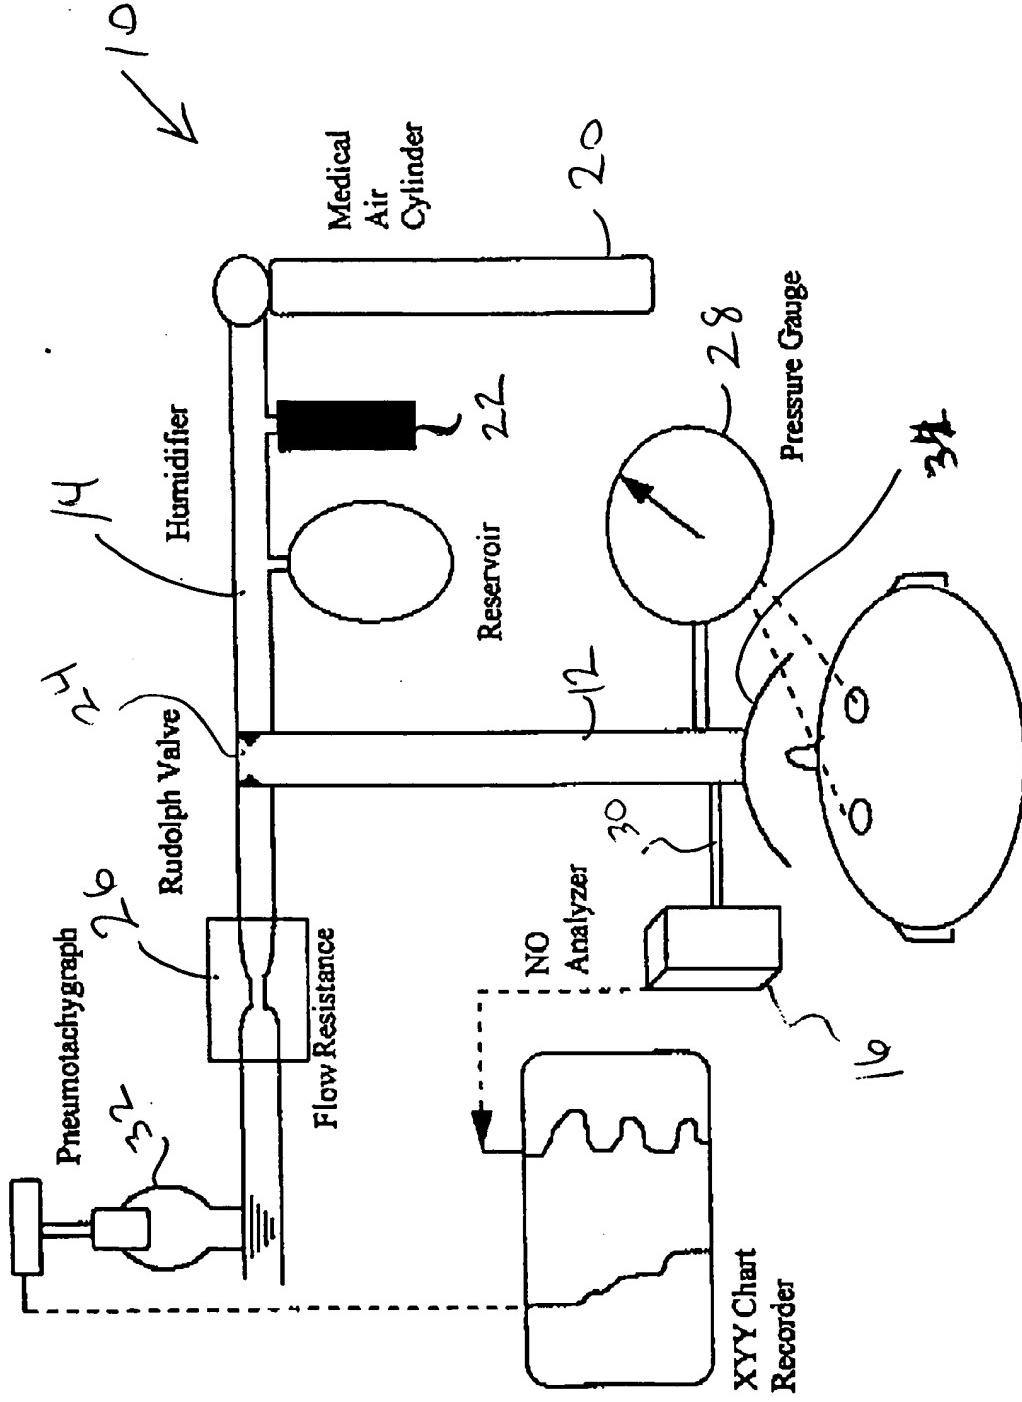


330
9-1

APPARATUS FOR EXHALED NO MEASUREMENTS

Figure 1.



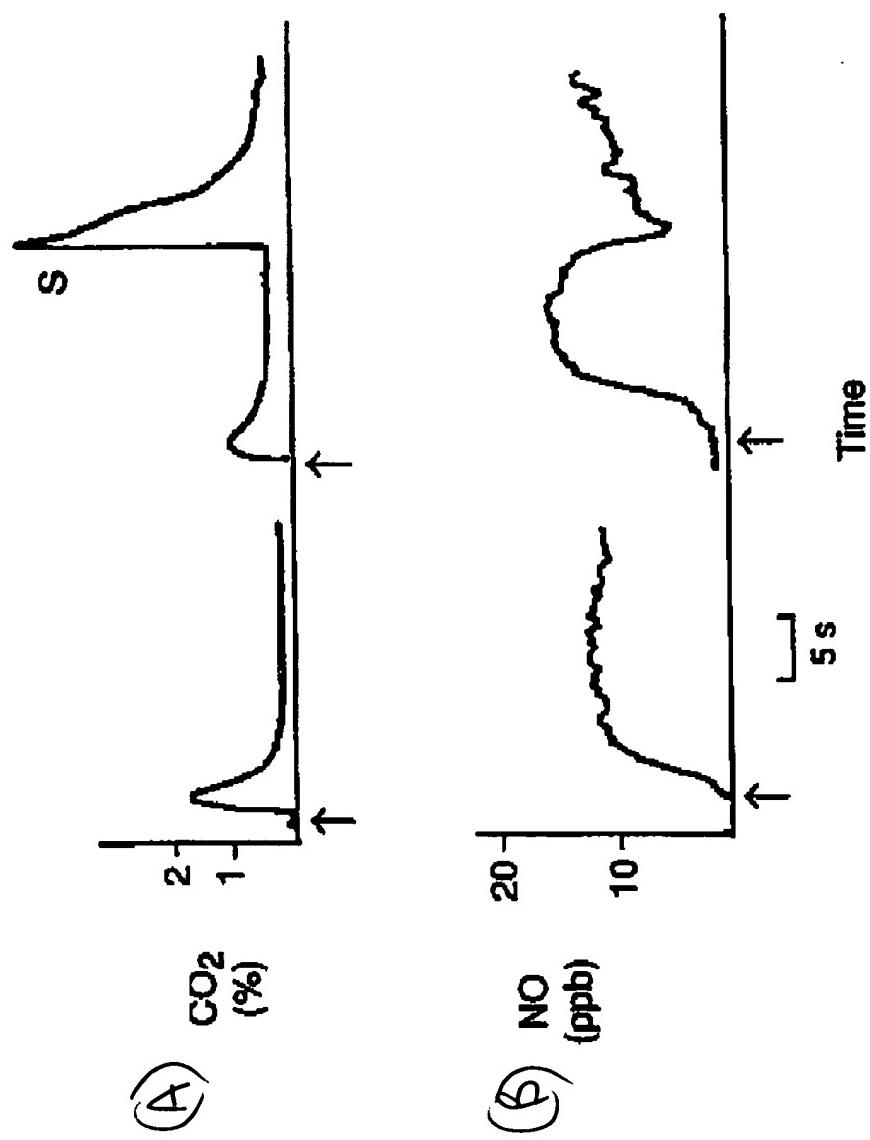


FIGURE 3



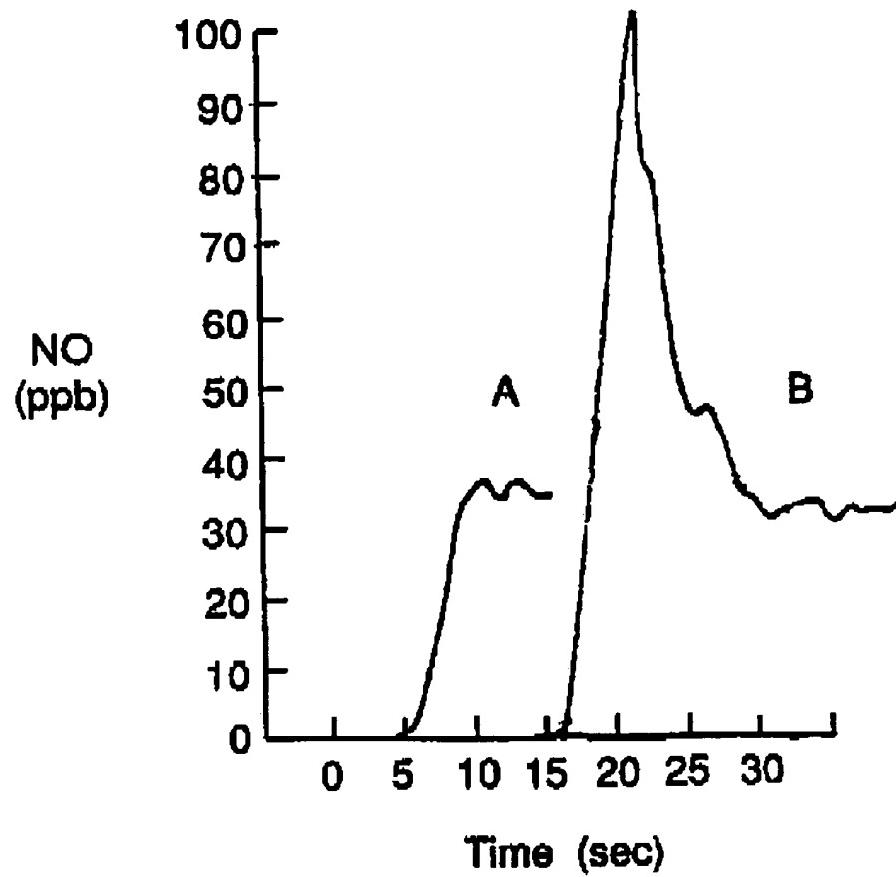


Fig 4a

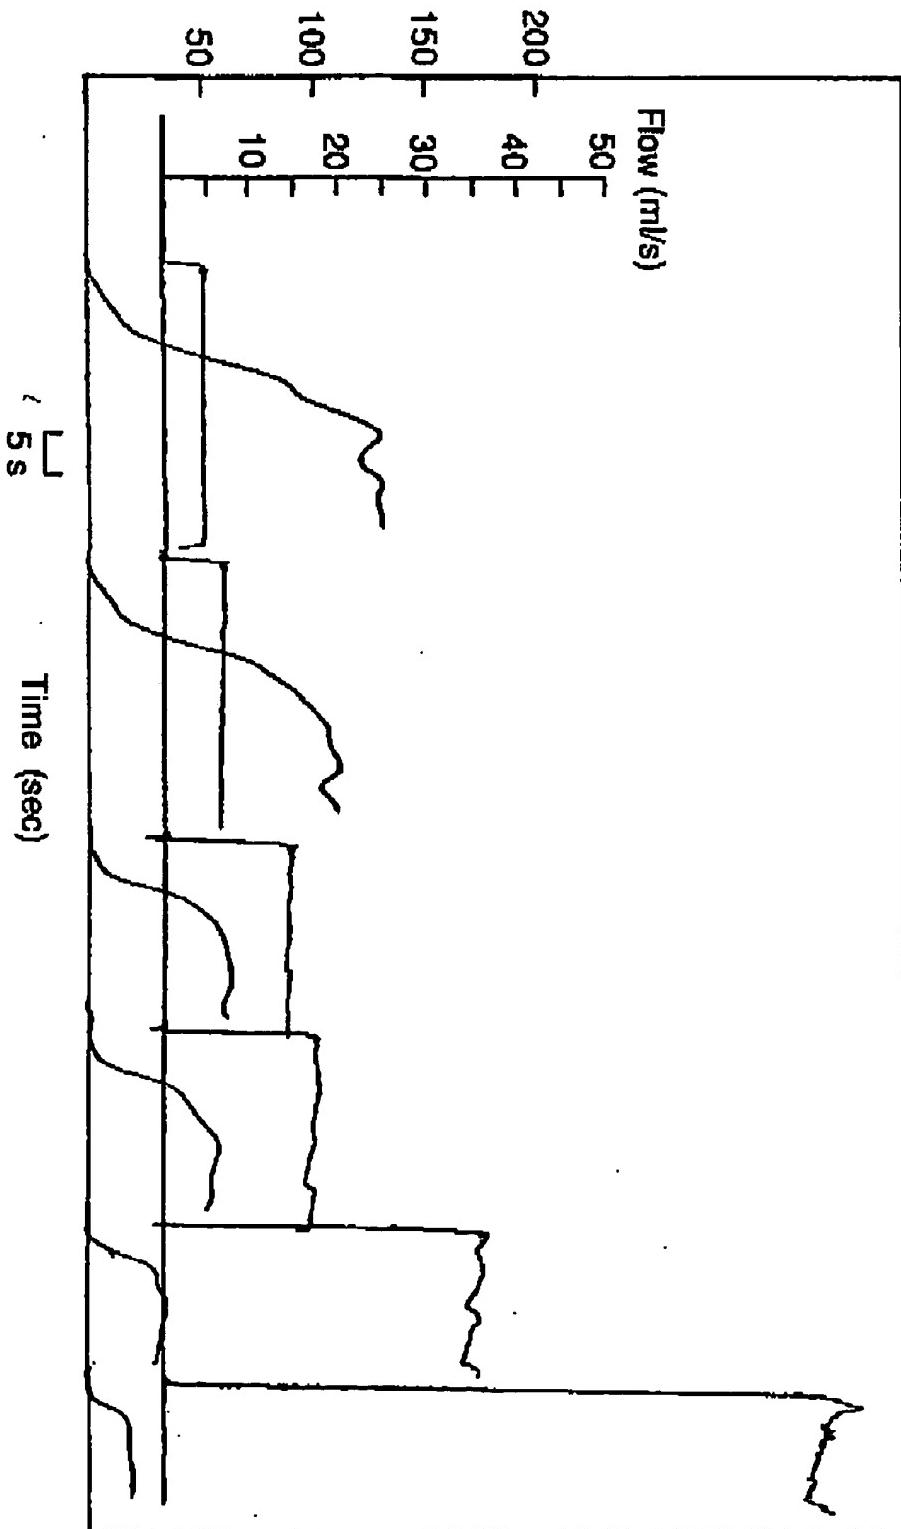


0 3 8 2 7 7 0 3 0 0 4 0 5 0 7


F1646

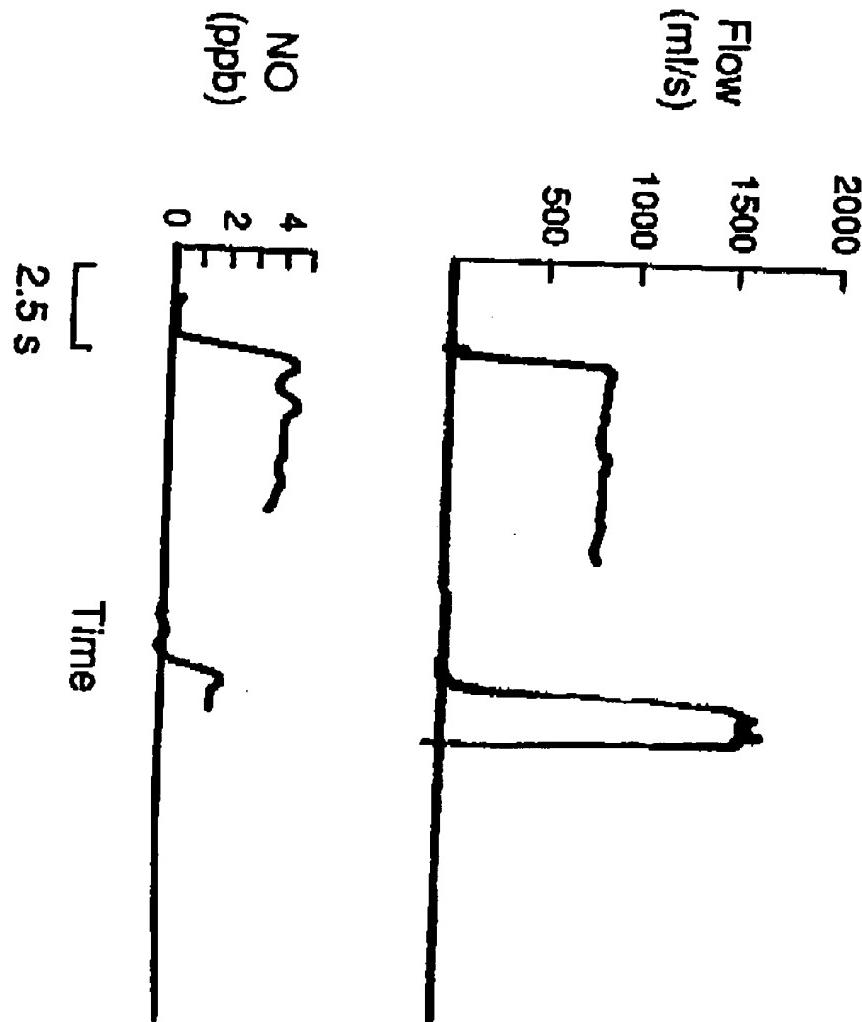


03327703 03460997

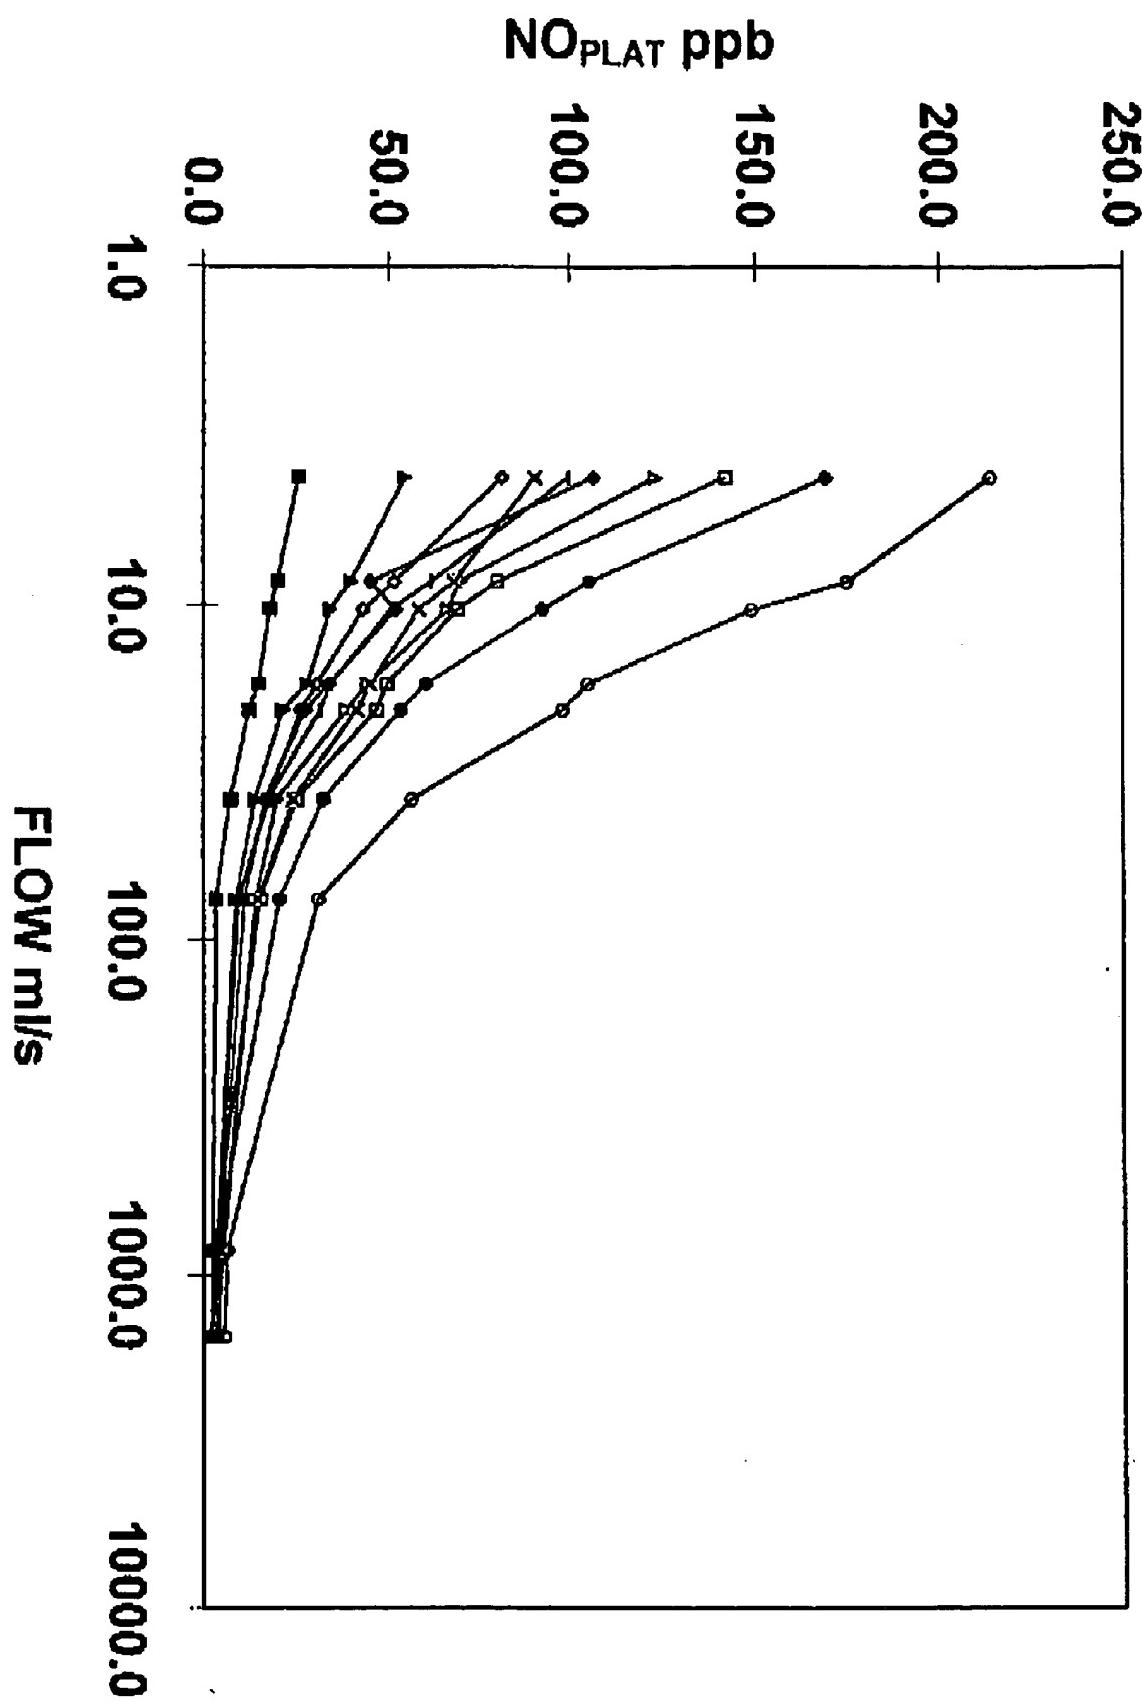

NO_{PLAT} % lowest flow
(\pm s.e.m)

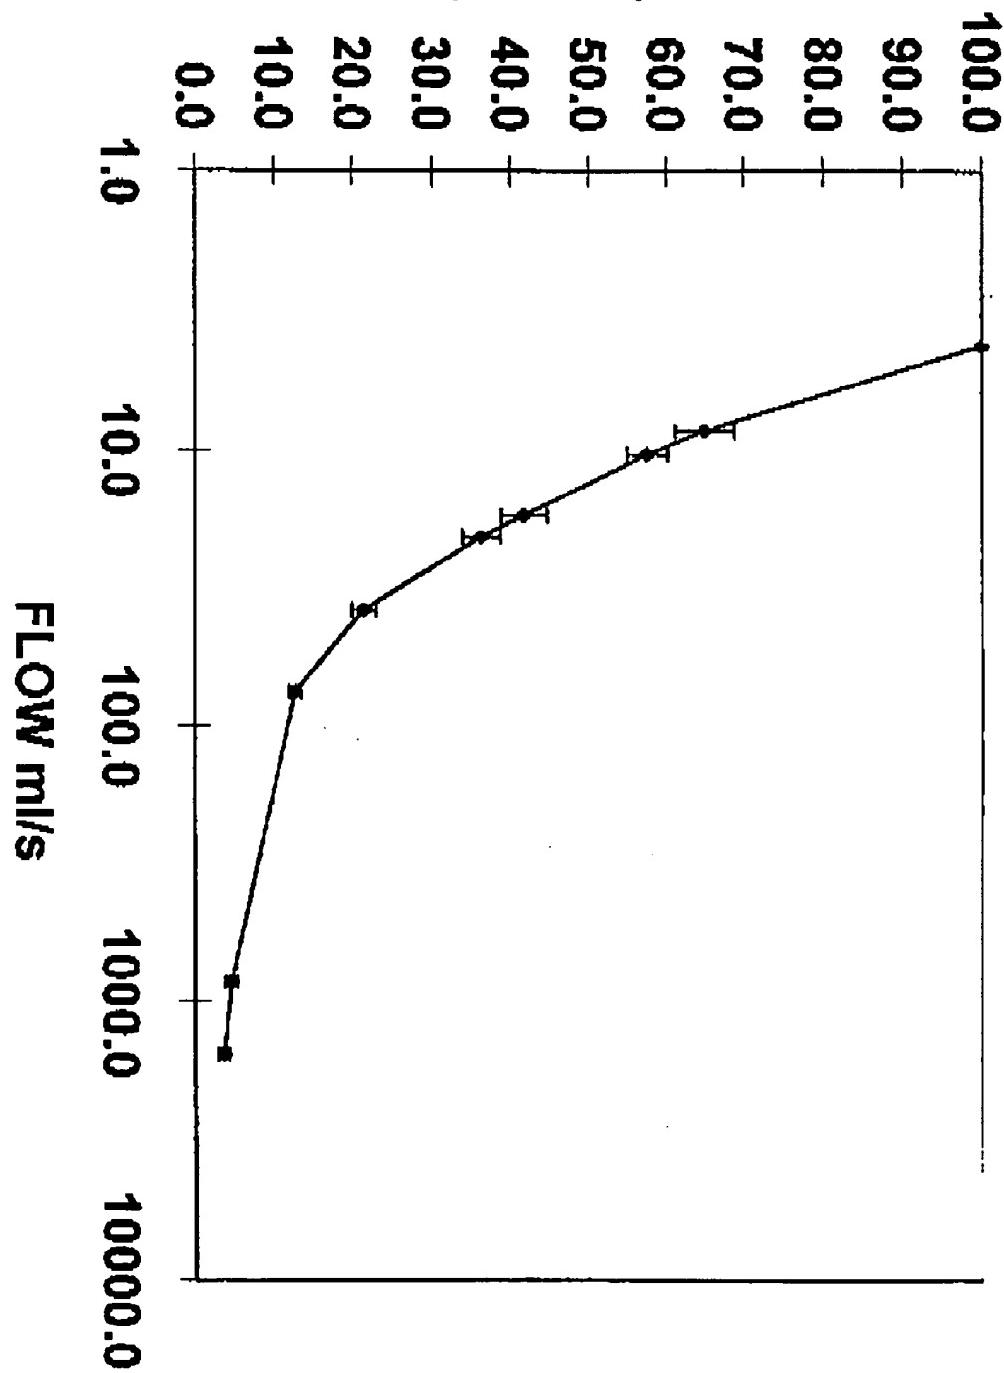

FIC-56-

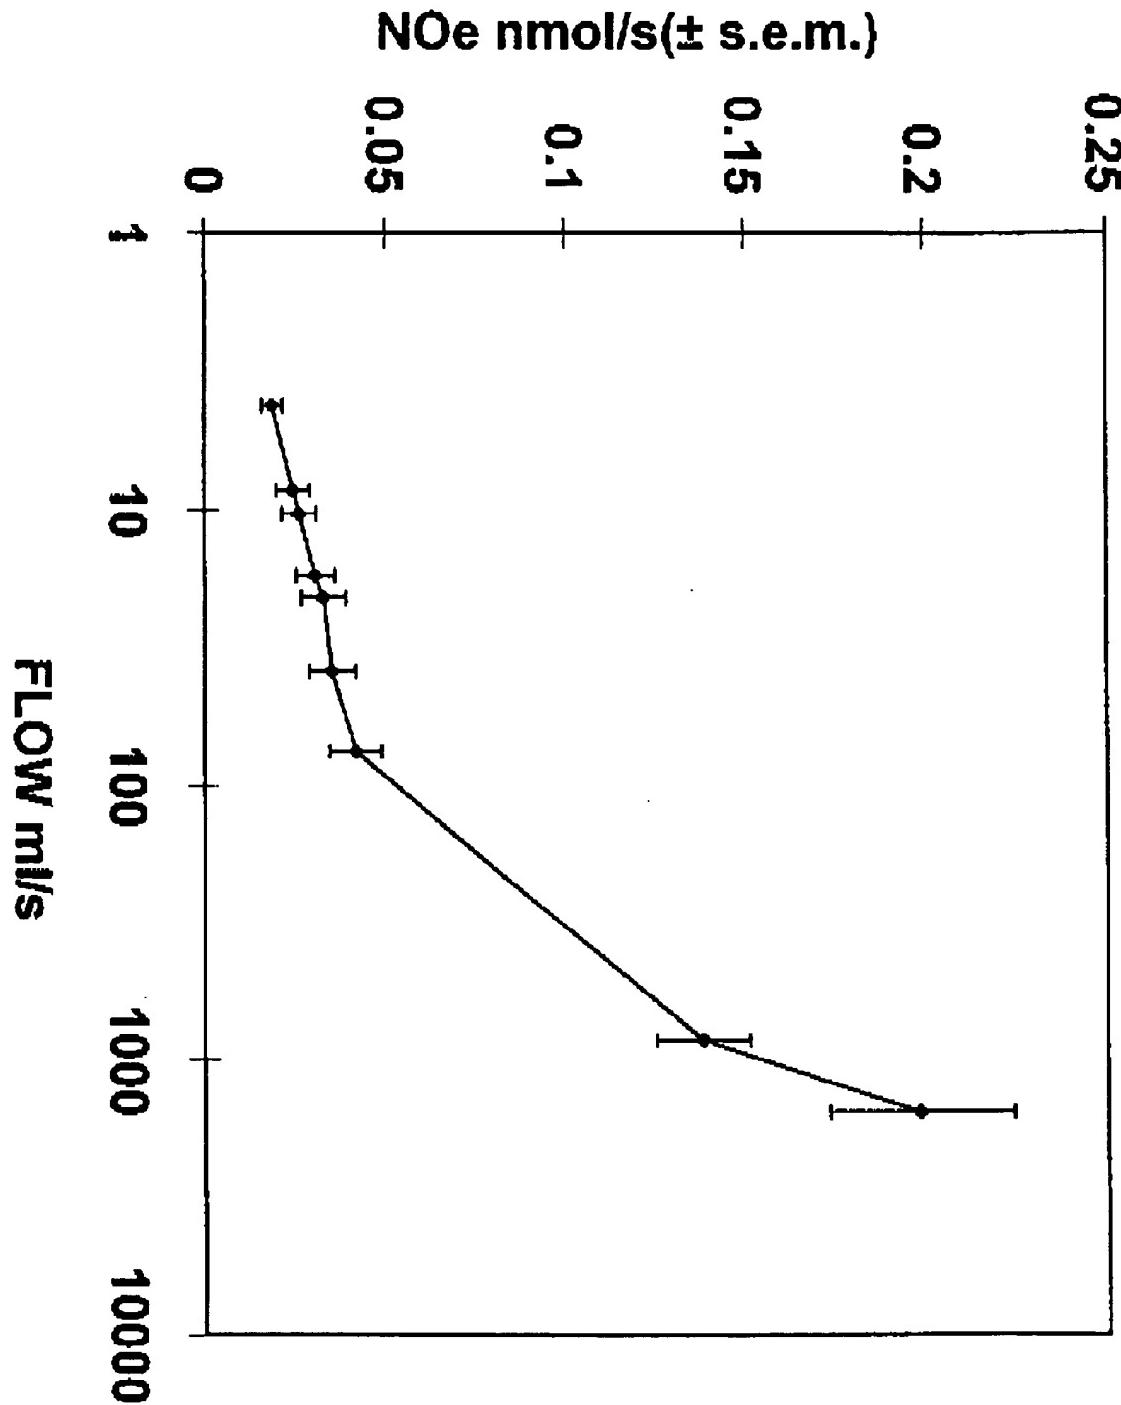

08627403 040997

JTC-6.

**REDUCED
HAEM.**

FIG 7

